

PRO EC Portable Meter MW302



CERTIFICATION

MW302 Instruments conform to the CE European Directives. Disposal of Electrical & Electronic Equipment. Do not treat this product as household waste. Hand it over to the appropriate collection point for the recycling of electrical and electronic equipment.

Disposal of waste batteries.

This product contains batteries. Do not dispose of them with other household waste. Hand them over to the appropriate collection point for recycling. Please note: proper product and battery disposal prevents potential negative consequences for human health and the environment. For detailed information, contact your local household waste disposal service.

RECOMMENDATION

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any modification introduced by the user to the supplied equipment may compromise the meter's performance. For your and the meter's safety do not use or store the meter in hazardous environment. To avoid damage or burn, do not perform any measurement in microwave ovens.

DESCRIPTION

This practical and ergonomic conductivity meter is ideal for anyone who works on a small budget and wants fast and reliable measurements for water analysis.

The MW302 PRO conductivity meter is a compact microprocessor-based device with a long service life.

This portable conductivity meter with automatic temperature compensation has an ergonomic case with a large LCD display that makes it easy to read the measurement.

Each set comes with a black cardboard box which includes:

- An MW302 conductivity meter
- An SE-520 conductivity probe (1 meter of cable)
- A calibration solution M10031B (1413 $\mu\text{S}/\text{cm}$, 20 mL)
- 1 x 9V alkaline battery
- A manual user



BAMO INTERNATIONAL

22, Rue de la Voie des Bans · Z.I. de la gare · 95100 ARGENTEUIL

Tel +33 (0)1 30 25 83 20 Web www.bamo.eu

Fax +33 (0)1 34 10 16 05 E-mail export@bamo.fr

PRO EC Portable Meter MW302

20-02-2023

M-372.02-EN-AB

RES


372-02/1

SPECIFICATIONS

Range/Résolution	0.0 to 10.0 mS/cm / 0.1 mS/cm
Accuracy	±2% Full Scale
Calibration solution	1413 µS/cm = 1.41 mS/cm (M10031B)
Conductivity sensor	SE-520 (included)
Temp. Compensation	Automatic, from 5 to 50°C
Environment	0 to 50 °C, 95% RH max.
Battery Type	1 x 9V alkaline (included)
Battery Life	Approximately 300 hours of use
Dimensions	143 x 80 x 32 mm
Weight	220 g (with battery) meter only

OPERATION

- The meter is supplied complete with a 9V battery.
- Slide off the battery compartment cover on the back of the meter. Install the battery into the battery clip connector while observing polarity.
- Connect the probe to the meter securely by aligning the pins with the plug in.
- Make sure that the meter has been calibrated before taking any measurements (see Calibration Procedure).
- Immerse the tip (4 cm) of the EC/TDS probe into the sample. If possible use plastic beakers or containers to minimize any EMC interference.
- Turn the instrument on by pressing the ON/OFF key.
- Wait for the temperature sensor to reach the thermal equilibrium before taking any measurements.
- After use, the instrument should be switched off and the probe should be cleaned and dried. Whenever needed, use alcohol for better cleaning.

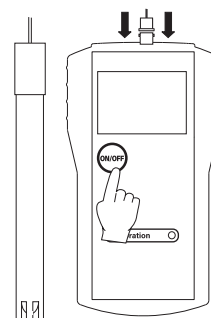

CALIBRATION PROCEDURE

- Clean the probe with alcohol and let it dry.
- Open a sachet of conductivity calibration solution (see Specifications) and immerse the probe making sure that the metal pins are completely submerged.
- Wait until the thermal equilibrium is reached and the reading is stable.
- Adjust the calibration trimmer on the front panel of the instrument with the supplied screwdriver until the display shows "1410 µS"
- The calibration is now complete and the meter is ready for use.



The instrument should be re-calibrated at least once a month, or whenever the probe or battery is changed

BATTERY REPLACEMENT

When the battery becomes weak the meter will display " ". When the low battery indicator appears, the battery has only about 50 hours of working time left. A low battery will result in unreliable measurements. Prompt battery replacement is required. Il est nécessaire de remplacer rapidement la pile.

Battery replacement must only take place in a non-hazardous area using an alkaline 9V battery.

Turn the meter off, slide the battery compartment cover located at the rear of the meter off and replace the 9V battery with a new one. Make sure the battery contacts are fully engaged in the connector, seat the battery in its compartment and replace the cover.

OPTIONAL ACCESSORIES

M10031B 1413 µS/cm (1.41 mS/cm) calibration solution, 20 mL sachet (25 pcs)

BAMO INTERNATIONAL

22, Rue de la Voie des Bans · Z.I. de la gare · 95100 ARGENTEUIL

Tel +33 (0)1 30 25 83 20 Web www.bamo.eu

Fax +33 (0)1 34 10 16 05 E-mail export@bamo.fr

**PRO EC Portable Meter
MW302**

20-02-2023

M-372.02-EN-AB

RES

372-02/2